



מדינת ישראל
STATE OF ISRAEL

10/522545
PCT/IL 03/00609
10 Res. CT/PTO 27 JAN 2005
REC'D 18 SEP 2003
WIPO PCT

Ministry of Justice
Patent Office

משרד המשפטים
לשכת הפטנטים

This is to certify that
annexed hereto is a true
copy of the documents as
originally deposited with
the patent application
of which particulars are
specified on the first page
of the annex.


זאת לתעודה כי
רצופים בזה העתקים
נכונים של המסמכים
שהופקדו לכתחילה
עם הבקשה לפטנט
לפי הפרטים הרשומים
בעמוד הראשון של
הנספח.

BEST AVAILABLE COPY

**PRIORITY
DOCUMENT**
SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

This 28-07-2003 היום

רשם הפטנטים
Commissioner of Patents

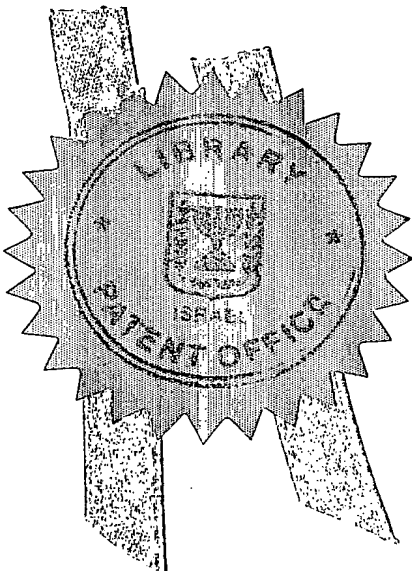

נתאשר
Certified

לשימוש הלשכה
For Office Use

| | |
|--------------------------------|------------|
| מספר: Number | 151029 |
| תאריך: Date | 01-08-2002 |
| הוקדם/נדחה: Ante/Post-dated | |

בקשה לפטנט
Application For Patent

אני, (שם המבקש, מענו ולגבי גוף מאוחד - מקום התאגדותו)
I, (Name and address of applicant, and in case of body corporate-place of incorporation)

אי.אר.טי מדיקל אינסטרומנטס בע"מ, השחר 33, הוד השרון 45325 (חברה ישראלית)
ART Medical Instruments Ltd, Hashahar 33, 45325 Hod Hasharon (an Israeli Company)


בעל אמצאה מכוח
Owner, by virtue of
העברה
Assignment
ששמה הוא
of an invention the title of which is

פד מסנן המסייע לגילוי נוכחות של פעולה פיסיולוגית, ושיטה עבורה, והתקן
לניטור תנועות עובר
(בעברית)
(Hebrew)

Bio-filter pad for facilitating the detection of an occurrence of a physiological
action, and method therefor, and fetal activity monitoring apparatus
(באנגלית)
(English)

Hereby apply for a patent to be granted to me in respect thereof.

מבקש בזאת כי ינתן לי עליה פטנט

| * בקשת חלוקה * | | * בקשת פטנט מוסף * | | זרישת דין קדימה | | |
|--|------|--------------------------------|------|--|---------------|------------------------------------|
| Application of Division | | Appl. for Patent of Addition | | Priority Claim | | |
| מבקשת פטנט from application | | לבקשה/לפטנט to Patent/Appl. | | מספר/סימן Number/Mark | תאריך Date | מדינת האירוע Convention Country |
| No. | מס' | No. | מס' | | | |
| Dated | מיום | Dated | מיום | | | |
| * יפוי כח: כללי / מיוחד - רצוף בזה / עוד יוגש P.O.A.: general / specific - attached / to be filed later - הוגש בענין _____ | | | |  | | |
| המען למסירות מסמכים בישראל Address for Service in Israel ART Medical Instruments Ltd. P.O.B 25290 61251 Tel Aviv | | | | | | |
| חתימת המבקש Signature of Applicant אי.אר.טי. מדיקל אינסטרומנטס בע"מ | | | | | | |
| | | | | שנת Year | July | בחודש of |
| | | | | 2002 | | 29 |
| | | | | היום This day | | |
| | | | | לשימוש הלשכה For Office Use | | |

This form, impressed with the Seal of the Patent Office and indicating the number and date of filing, certifies the filing of the application the particulars of which are set out above.

* מחק את המיותר
Delete whatever is inapplicable

פד מסנן המסייע לגילוי נוכחות של פעולה פיסיולוגית, ושיטה
עבודה, והתקן לניטור תנועתיות עובר

Bio-filter pad for facilitating the detection of an occurrence of a
physiological action, and method therefor, and
fetal activity monitoring apparatus

BIO-FILTER PAD FOR FACILITATING THE DETECTION OF AN OCCURRENCE OF A PHYSIOLOGICAL ACTION, AND METHOD THEREFOR, AND FETAL ACTIVITY MONITORING APPARATUS

Field of the Invention

5 The invention is in the field of medical diagnostic apparatus and methods for detecting an occurrence of a physiological action in general, and fetal activity in particular.

Background of the Invention

10 Fetal activity has long been recognized as a good predictor of fetal well being as discussed in Fetal Movements In utero – A Review, Sadovsky, E., M.D., Isr. J. Obstet. Gynecol. 1992; 3:27-36. Fetal activity monitoring techniques run the gamut from an expectant mother's subjective assessment of fetal activity via fetal activity monitoring apparatus for monitoring her abdominal movements to *in utero* ultrasound based techniques for "*looking inside*" her uterus. Fetal
15 activity monitoring apparatus is designed to monitor an expectant mother's abdominal movements within the range of 8-25 Hz which is the natural frequency signature of an expectant mother's abdomen. Such abdominal movements are assumed to be largely the result of fetal activity as opposed to uterine contractions, respiratory movements, maternal posture movements, and
20 the like, and therefore the 8-25 Hz natural frequency signature of an expectant mother's abdomen is hereinafter coined as "*natural fetal activity frequency signature*".

 An exemplary fetal activity monitoring apparatus is described in an article entitled "Measurement of Fetal Movements by Moving-Coil Transducer" by
25 Adler D., et al., IEEE Transactions on Biomedical Engineering, Vol. BME-27, No. 12, December 1980 which employs two moving-coil transducers placed on the left and the right sides of an expectant mother's abdomen to pick up abdominal movements. This apparatus requires an about 80 dB electrical signal

amplification for fetal activity detection at least partially being necessitated to overcome the transducers' attenuation of frequencies in the natural fetal activity frequency signature, and offset the apparatus' high sensitivity to electro-magnetic interference (EMI).

5 Summary of the Invention

Generally speaking, the present invention is directed toward a bio-filter pad capable of physically amplifying displacements within the range of a natural frequency signature associated with an occurrence of a physiological action for facilitating detection of such an occurrence. This is achieved by the bio-filter pad
10 having a mechanical resonance frequency preferably midway in the range of the natural frequency signature, and a transducer for intimate mechanical coupling therewith also preferably tuned to the same mechanical resonance frequency to increase physical amplification of a displacement, thereby lessening electrical signal amplification requirements by a suitable physiological activity recorder.

15 At the present time, it is envisaged that the primary application of the present invention will be for fetal activity monitoring purposes in general, and home based fetal activity monitoring purposes in particular but it is also envisaged that the bio-filter pad of the present invention can be adapted for use in sport medicine, rehabilitation, and the like. For fetal monitoring purposes, a bio-
20 filter pad and a transducer preferably each have the same mechanical resonance frequency midway in the range of the natural fetal activity frequency signature whereby they are capable of yielding from about 20 to about 50 physical amplification of an abdominal displacement. By virtue of this physical amplification, a suitably tuned transducer and a fetal activity recorder together
25 constituting fetal activity monitoring apparatus need only a combined about 45 dB electrical signal amplification as opposed to the hitherto required 80 dB electrical signal amplification in the above-mentioned Adler article, thereby also inherently beneficially reducing the latter's EMI sensitivity.

Brief Description of the Drawings

In order to understand the invention and to see how it can be carried out in practice, preferred embodiments will now be described, by way of a non-limiting example only, with reference to the accompanying drawings in which similar parts are likewise numbered, and in which:

Fig. 1 is a schematic representation of a first preferred embodiment of a fetal activity monitoring system in accordance with the present invention including a bio-filter pad, a transducer and a fetal activity recorder;

Fig. 2 is a graph showing the natural fetal activity frequency signature of an expectant mother's abdomen;

Fig. 3 is a pictorial representation of the bio-filter pad of Figure 1;

Fig. 4 is a longitudinal cross section view of the bio-filter pad of Figure 1 along line A-A in Figure 3;

Fig. 5 is a graph showing the transmissibility response curve of the bio-filter pad of Figure 1; and

Fig. 6 is a schematic representation of a second preferred embodiment of a fetal activity monitoring system in accordance with the present invention.

Detailed Description of Preferred Embodiments

Figure 1 shows a fetal activity monitoring system 1 suitable for home use for providing a visual indication regarding the prevailing level of fetal activity based on detecting an expectant mother's abdominal movements having a typical natural fetal activity frequency signature FS (see Figure 2). The fetal activity monitoring system 1 includes a bio-filter pad 2 adapted for removable intimate adhesion to her abdomen, and having a moving coil transducer 3 centrally disposed thereon for picking up her abdominal movements. The transducer 3 is connected to a credit-card like, battery powered, fetal activity recorder 4 having an amplifier 6, an A/D converter 7, a signal processor 8, a memory 9, an output interface 11, for example, RS-232, and a fetal activity display 12 for comparing the prevailing fetal activity during a fetal activity monitoring session to a regular

level of fetal activity determined on the basis of historical information. The fetal activity display 12 has three LEDs: a green LED 13 for indicating a regular level of fetal activity, an orange LED 14 for indicating a marginally lower than regular level of fetal activity, and a red LED 16 for indicating a significantly lower than regular level of fetal activity. The transducer 3 and the fetal activity recorder 4 have a combined electrical signal amplification in the order of about 45 ± 5 dB.

Figure 3 shows that the bio-filter pad 2 has a topside 17 formed with a resiliently elastic restraining member 18 for intimately mechanically coupling the transducer 3 to the bio-filter pad 2 on its being slid thereunder, and an underside 19 with a peel-off protective liner 21 for exposing an adhesive surface 22 enabling the removable intimate adhesion of the bio-filter pad 2 to an expectant mother's abdomen. The bio-filter pad 2 is preferably circular with a diameter within the range of about 10 cm to about 25 cm, and has a thickness within the range of about 1 mm to about 5 mm. The bio-filter pad 2 has a vascoelastic interior 23 with concentric sections for focusing mechanical energy imparted thereto due to abdominal movements for enabling detection of most if not all fetal activity and not just limb movements directed towards the transducer 3 (see Figure 4). The viscoelastic interior 23 may be constituted by a solid material, or a fluid material, or a combination thereof. The bio-filter pad 2 has a 12 Hz mechanical resonance frequency for physically amplifying displacements within the natural frequency fetal activity signature (see Figure 5), as does the transducer 3. The mechanical resonance frequencies of the bio-filter pad 2 and the transducer 3 can be tested by knocking on them. The mechanical coupling between the bio-filter pad 2 and the transducer 3 are such that they yield from about 20 to about 50 physical amplification of an abdominal displacement, thereby accentuating a natural fetal activity frequency signature.

The fetal activity monitoring system typically replaces an expectant mother's subjective assessment of fetal activity in an otherwise conventional fetal activity monitoring program. Thus, in accordance with her fetal activity

monitoring program, she removes a peel-off protective liner from a bio-filter pad, intimately adheres the bio-filter pad onto her abdomen, couples the transducer to the bio-filter pad, and proceeds to record her abdominal movements. In the normal course of events, the green LED will be illuminated and no special action need to be taken. In the event that either the yellow LED or red LED is illuminated during a fetal activity monitoring session, she takes the fetal activity recorder storing all historical fetal activity information to a medical specialist for a professional diagnosis.

Figure 6 shows a fetal activity monitoring system 31 similar to the fetal activity monitoring system 1 except that instead of its fetal activity recorder 32 being a standalone unit, it is intended for removable attachment to a mobile telephone 33 for both being powered thereby, and for connection to a remote server 34 for data processing purposes. To this end, the fetal activity recorder 32 includes a data compression processor 36 for compressing a fetal activity recording for selective transmission to the remote server 34, and an audio output 37 for connection to the mobile telephone's audio input. The results of a fetal activity monitoring session are preferably transmitted by SMS for display on the mobile telephone's display 38.

While the invention has been described with respect to a limited number of embodiments, it will be appreciated that many variations, modifications, and other applications of the invention can be made within the scope of the appended claims. For example, the bio-filter pad may be oval shaped, and employ different restraining techniques for juxtaposing a transducer against its topside, and the like.

Claims:

1. For use in the detection of an occurrence of a physiological action imparting a displacement to a body part at a natural frequency signature, a bio-filter pad comprising a viscoelastic interior for intimate juxtapositioning against the body part, and having a mechanical resonance frequency midway in the range of the frequency signature associated with the physiological action.
2. The pad according to claim 1 further comprising a peel-off protective liner for exposing an adhesive surface suitable for removable intimate adhesion of the bio-filter pad onto the body part.
3. The pad according to either claim 1 or 2 wherein said viscoelastic interior has concentric sections for focusing mechanical energy imparted to the bio-filter pad due to a displacement of the body part lying thereunder toward a transducer centrally disposed on its topside facing away from the body part.
4. The pad according to any one of claims 1 to 3 and further comprising a restraining member on its topside for removably intimately mechanically coupling a transducer to its topside.
5. The pad according to claim 4 wherein said restraining member slidably receives said transducer.
6. The pad according to any one of claims 1 to 5 wherein the bio-filter pad is sized and shaped for conforming to an expectant mother's abdomen, and has a mechanical resonance frequency midway in the natural fetal activity frequency signature for fetal activity monitoring purposes.

7. The pad according to any one of claims 1 to 6 wherein the bio-filter pad is intended for single patient single use.

8. A method for detecting an occurrence of a physiological action
5 imparting a displacement to a body part at a natural frequency signature, the method comprising the steps of:

(a) intimately juxtaposing a bio-filter pad against
the body part, the bio-filter pad having a viscoelastic
interior, and a mechanical resonance frequency
10 midway in the range of the natural frequency
signature associated with the physiological action;

(b) intimately mechanically coupling at least one
transducer against the topside of the bio-filter pad for
generating electrical signals in response to
15 displacements of the body part; and

(c) processing the electrical signals for detecting
occurrences of the physiological action.

9. The method according to claim 8 wherein step (a) includes the step of
20 removing a peel-off protective liner from the underside of the bio-filter pad
exposing an adhesive surface for removable intimate adhesion of the bio-filter
pad onto the body part.

10. The method according to either claim 8 or 9 wherein step (b) includes
25 removably sliding the transducer under a restraining member on the topside of
the bio-filter pad.

11. The method according to any one of claims 8 to 10 and further
comprising the step of focusing mechanical energy imparted to the bio-filter pad
30 due to a displacement of the body part lying thereunder toward the transducer.

12. The method according to any one of claims 8 to 11 wherein the bio-filter pad is sized and shaped for conforming to an expectant mother's abdomen, and has a mechanical resonance frequency midway in the natural fetal activity frequency signature for fetal activity monitoring purposes.

13. The method according to any one of claims 8 to 12 wherein the bio-filter pad is intended for single patient single use.

10 15. Fetal activity monitoring apparatus comprising at least one transducer for intimate juxtaposition against an expectant mother's abdomen for generating electrical signals in response to her abdominal movements; and a fetal activity recorder for processing the electrical signals for detecting occurrences of fetal activity,

15 characterized in that
the apparatus has an electrical signal amplification of about 45 ± 5 dB.

16. Apparatus according to claim 15 wherein said fetal activity recorder has an audio output for interfacing with a mobile telephone.

20 17. Apparatus according to claim 16 wherein said fetal activity recorder includes a data compression capability for transmitting compressed data via for remote processing.

25

Respectfully submitted,



A.R.T. Medical Instruments Ltd.

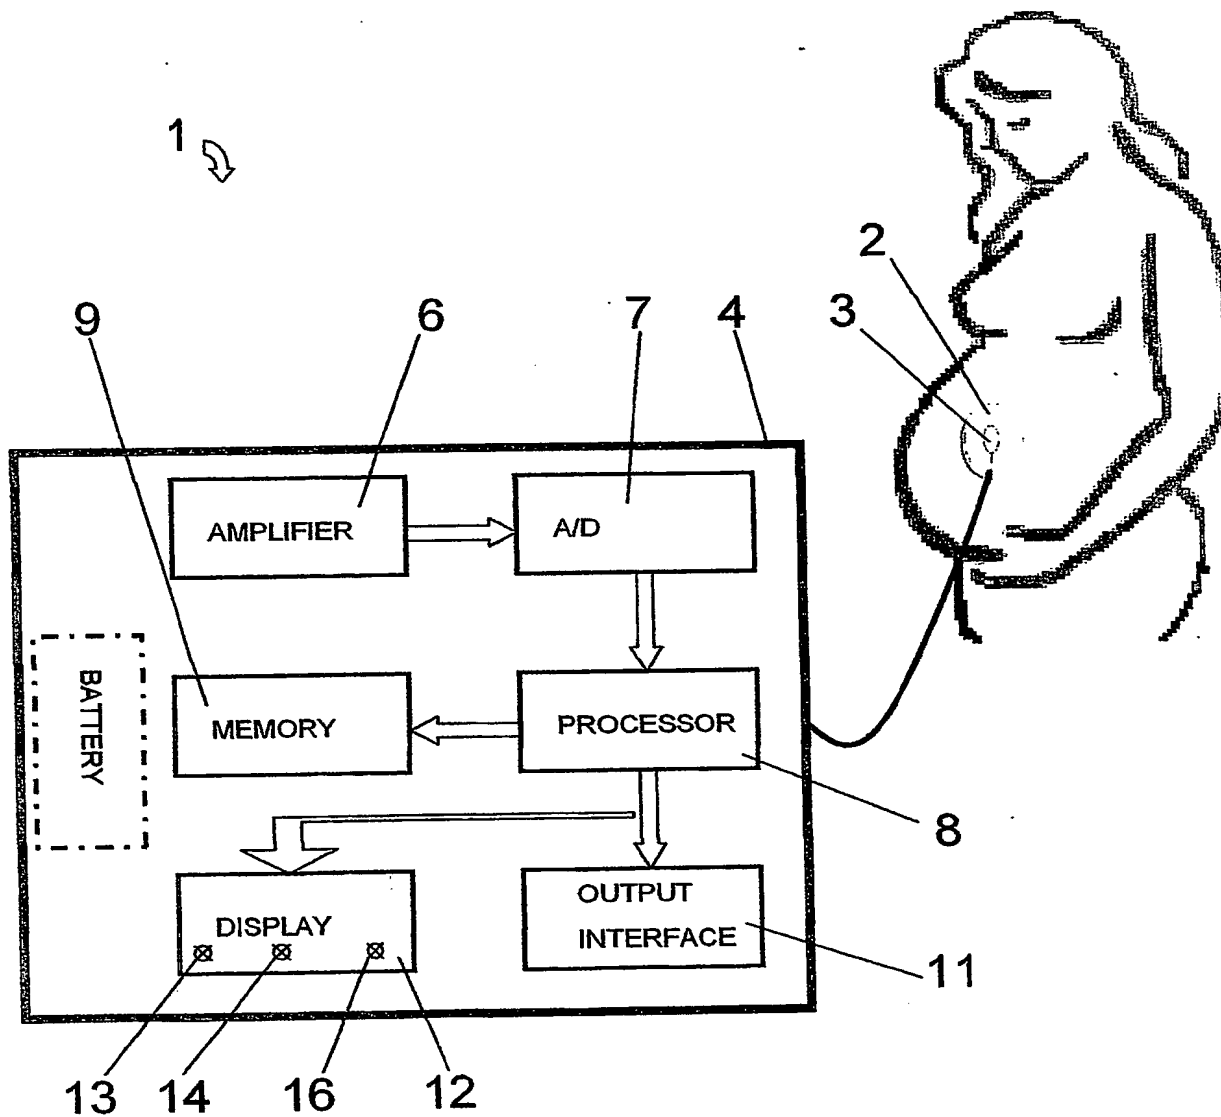


FIG. 1

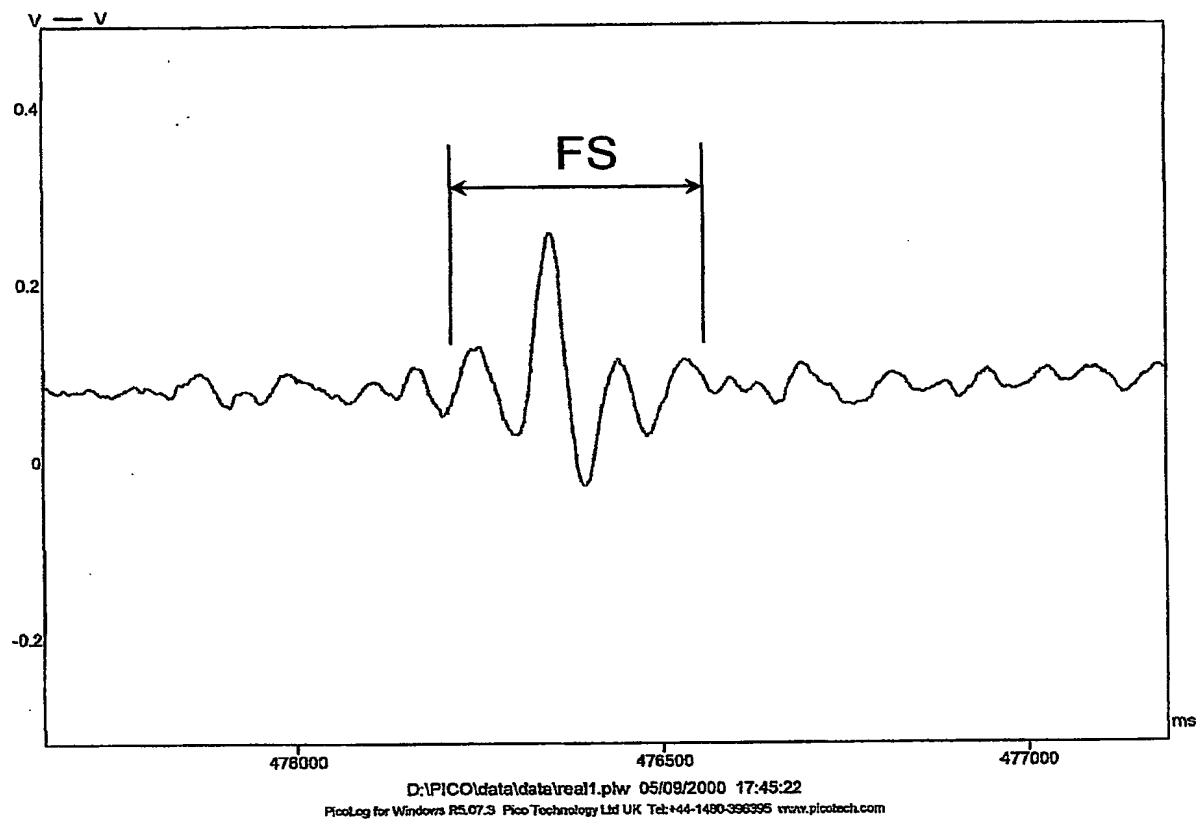


FIG. 2

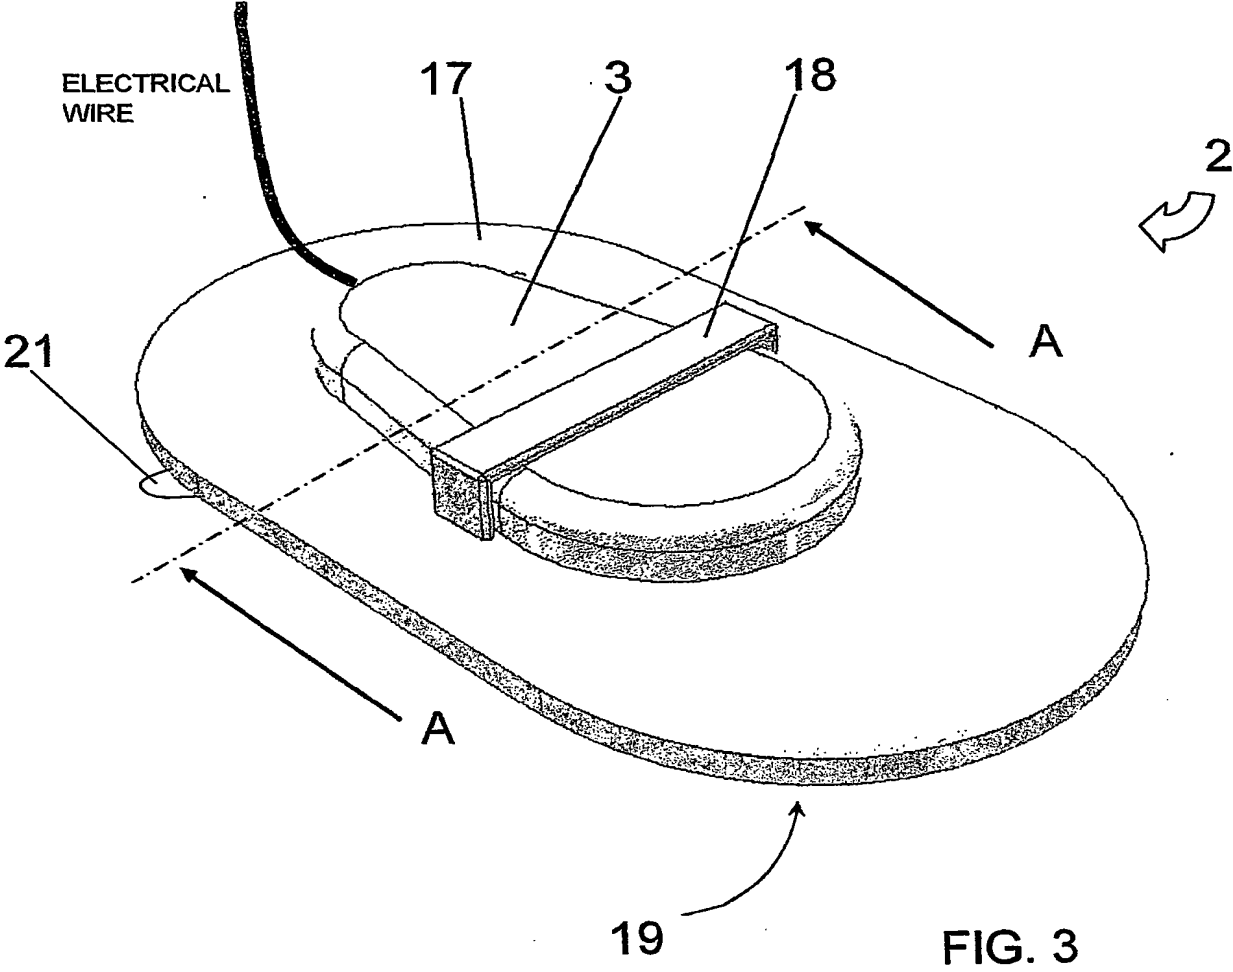


FIG. 3

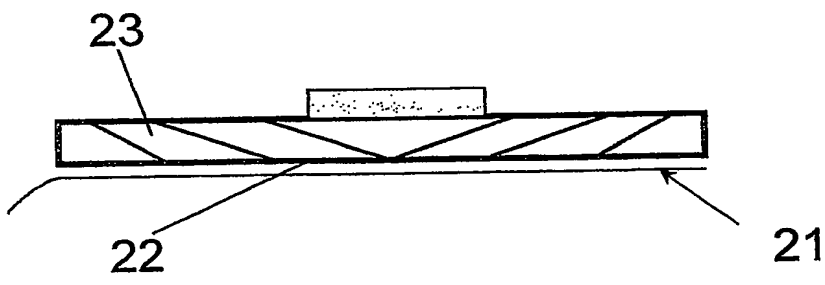


FIG. 4

AMPLIFICATION

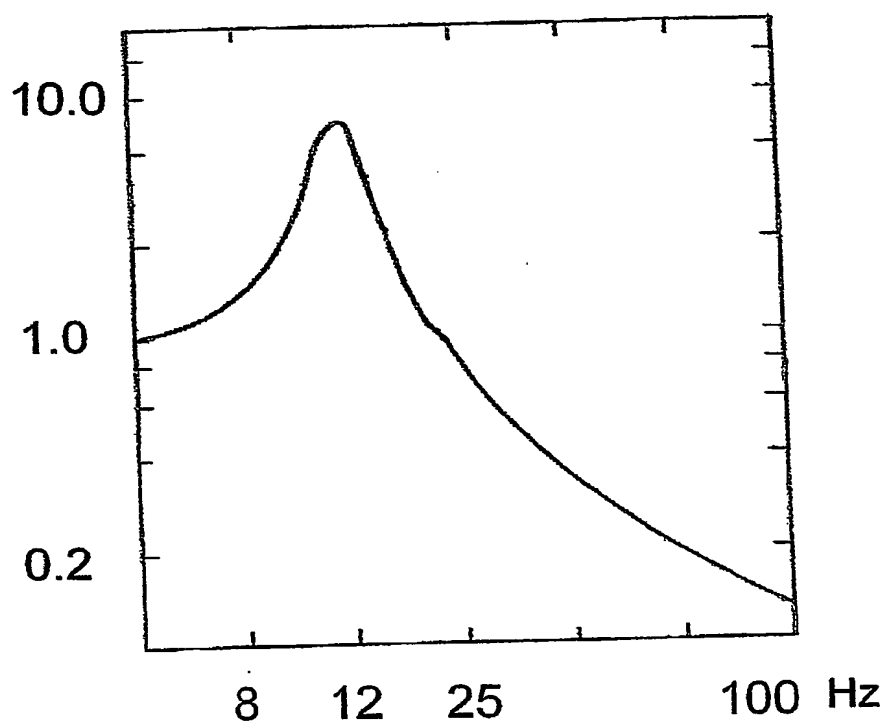


FIG. 5

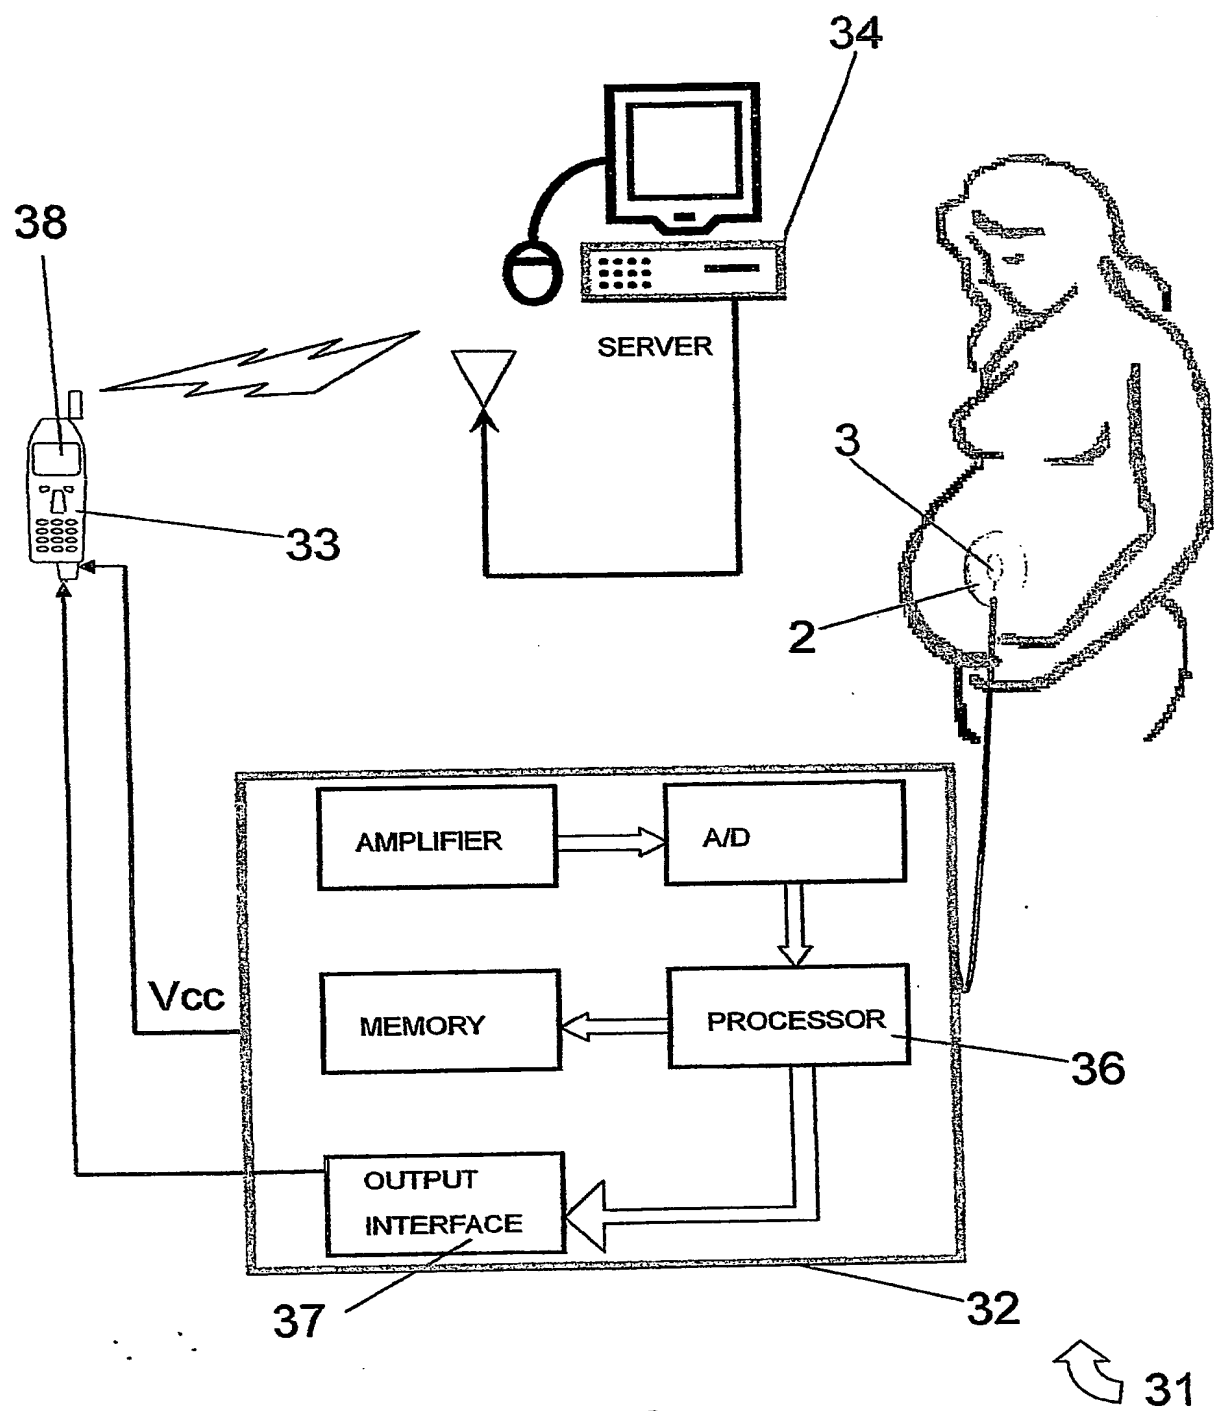


FIG. 6

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.